

INTEGRATED VISION-BASED SYSTEM FOR EFFICIENT, SEMI-AUTOMATED CONTROL OF A ROBOTIC MANIPULATOR

HAIRONG JIANG

*School of Industrial Engineering, Purdue University,
315 N. Grant Street, West Lafayette, IN47907, USA
jiang115@purdue.edu*

JUAN P. WACHS

*School of Industrial Engineering, Purdue University,
315 N. Grant Street, West Lafayette, IN47907, USA
jpwachs@purdue.edu
<http://web.ics.purdue.edu/~jpwachs/> >*

Bradley S. Duerstock*

*Weldon School of Biomedical Engineering,
School of Industrial Engineering, Purdue University,
206 S. Martin Jischke Drive, West Lafayette, IN47907, USA
bsd@purdue.edu
<http://web.ics.purdue.edu/~bsd/> >*

Received 23-Sept-2013

Revised 27-Feb-2014

Accepted 3-Mar-2014

Purpose- Develop an integrated, computer vision-based system to operate a commercial wheelchair-mounted robotic manipulator (WMRM). In addition, a gesture recognition interface system was developed specially for individuals with upper-level spinal cord injuries (SCIs) including object tracking and face recognition to function as an efficient, hands-free WMRM controller.

Design/Methodology/Approach- Two Kinect cameras were used synergistically to perform a variety of simple object retrieval tasks. One camera was used to interpret the hand gestures and locate the operator's face for object positioning, and then send those as commands to control the WMRM. The other sensor was used to automatically recognize different daily living objects selected by the subjects. An object recognition module employing the Speeded Up Robust Features (SURF) algorithm was implemented and recognition results were sent as a commands for "coarse positioning" of the robotic arm near the selected object. Automatic face detection was provided as a shortcut enabling the positing the objects close by the subject's face.

Findings- The gesture recognition interface incorporated hand detection, tracking and recognition algorithms, and yielded a recognition accuracy of 97.5% for an eight-gesture lexicon. Tasks' completion time were conducted to compare manual (gestures only) and semi-manual (gestures, automatic face detection and object recognition) WMRM control modes. The use of automatic face and object detection significantly reduced the completion times for retrieving a variety of daily living objects.

Originality/value- Integration of three computer vision modules were used to construct an effective and hand-free interface for individuals with upper-limb mobility impairments to control a WMRM.

Keywords Spinal cord injuries; gesture recognition; wheelchair-mounted robotic arm; object recognition.

Paper Type Research paper

1. Introduction

Previous studies have been conducted to develop wheelchair-mounted robotic manipulators (WMRMs) that provide persons with upper extremity mobility impairments, such as persons with upper-level SCIs, greater autonomy and less reliance on others in retrieving and manipulating objects for activities of daily living (ADL) (Amat, 1998; Chung and Cooper, 2012; Kim *et al.*, 2012).

The development of WMRMs has been facilitated by the availability of commercial robotic arms emerging in the market. For instance, the Manus manipulator, produced by Exact Dynamics® is a 6 degree of freedom (DoF) robotic manipulator that can be re-programmed and mounted to a wheelchair system (Eftring and Boschian, 1999). The JACO robotic arm developed by Kinova® is a light-weight robotic manipulator that is designed to be mounted to a motorized wheelchair to help people with upper limb impairments with ADL (Maheu *et al.*, 2011). However, these commercially-available systems are designed to be controlled by traditional modalities (i.e. joystick), which may not be usable by operators with upper extremity motor impairments.

Prior investigations in human-computer interaction (HCI) for persons with upper extremity motor impairments or quadriplegics has resulted in alternate user input options. The greatest advances have occurred in personal computer (PC) control utilizing speech recognition, facial expression, eye tracking, and hand gesture recognition (Jacko, 2011; Reale *et al.*, 2011). However, these HCI modalities, which do not rely upon switch or joystick operation, have also been useful for controlling actuated assistive technology (AT) devices, such as driving intelligent wheelchairs. Alternate input modalities that do not require switch, button or joystick operation for directly or semi-autonomously controlling intelligent wheelchairs include speech recognition (Nishimori *et al.*, 2007), gesture recognition (Reale *et al.*, 2011) tongue movement (Vaidyanathan *et al.*, 2007), or electromyography (EMG) and electrooculography (EOG) (Tsui *et al.*, 2007). More modalities can be combined for smart wheelchairs control. For example, facial gestures, EMG, and voice commands were integrated to control an intelligent wheelchair (Moon *et al.*, 2003). For an exhausted review of the literature in this field, refer to Simpson's review (Simpson, 2005).

These control modalities also have benefits for controlling robotic arms for WMRM systems, though the positioning of the robotic gripper in three-dimensional Cartesian space and prehensile manipulating of objects provide unique challenges. However, existing HCI modalities (Kim *et al.*, 2012) as well as emerging brain computer interfaces (BCI) (Palankar *et al.*, 2009) and state-of-the-art computer vision systems have been shown to be capable controllers for WMRM systems (Kim *et al.*, 2009; Tsui *et al.*, 2007). This latter work has shown that a camera mounted in the hand of the robotic manipulator provides an effective visual interface for WMRM control (Chung and Cooper, 2012; Kim *et al.*, 2012; Tsui *et al.*, 2011). Vision-based systems have become more popular for wheelchair navigation and WMRM control (Yanco, 2000). A vision-based system, named Wheeley, was developed to navigate a robotic wheelchair by interpreting the cues, such as building directories at entrances and room numbers (Bailey *et al.*, 2007; Yanco,

2000). A vision-based system was evaluated for use with the UCF-MANUS WMRM using a touchscreen interface. It was found equivalent to other input modalities but significantly better than the trackball operation (Kim *et al.*, 2012).

We developed an upper limb gesture recognition system to control a WMRM utilizing the JACO robotic arm. Hand and arm gestures are an intuitive communication form and provide an effective HCI modality. Gesture recognition does not require sensors or other contacts to the operator's body compared to other HCIs, such as EMG, EOG, tongue drives. Likewise, the user does not need to make contact with buttons, joysticks, touchscreens, or sip and puff straws allowing free arm movement during AT device control (Hashimoto *et al.*, 2009). Moreover, the lexicon of hand gestures for a gesture recognition-based interface can be customized to meet the requirements of the users for certain tasks. The works in (Wachs *et al.*, 2005) have shown that gestures are a simple and intuitive modality for robotic manipulator control. A comparison between our system and other similar state-of-the-art interfaces is shown in Table I.

Table I. Comparison with other interfaces

State of the art	Input modality	Wheelchair mounted robot manipulator (WMRM)	DoF	Vision	Setting
Wheeley (Bailey <i>et al.</i> , 2007)	Joystick	One WMRM (two-fingered gripper)	6	✓ Stereo camera (one)	Fixed on the wheelchair
Human-in-the-loop (Tsui <i>et al.</i> , 2011)	Joystick Touchpad	One WMRM (two-fingered gripper)	6	✓ Stereo camera (two)	Fixed on the wheelchair
PerMMA (Wang <i>et al.</i> , 2012)	Joystick Touch screen	Two WMRMs (two-fingered gripper)	6	✓ Web camera (two)	Fixed on the wheelchair
Assistive Robot (Kim <i>et al.</i> , 2012)	Touch screen Trackball Microphone and jelly switch Trackball and jelly switch	One WMRM (two-fingered gripper)	6	✓ Stereo camera (one)	Fixed on the wheelchair
Robotic smart house (Park <i>et al.</i> , 2007)	Hand gesture Voice Body movement Posture	Robotic hoist Intelligent bed and wheelchair	--	✓ Web Camera (three)	Standalone
Our system	Hand gesture Automatic object recognition	One WMRM (three-fingered gripper)	6	✓ 3D sensors (two)	Fixed on the wheelchair

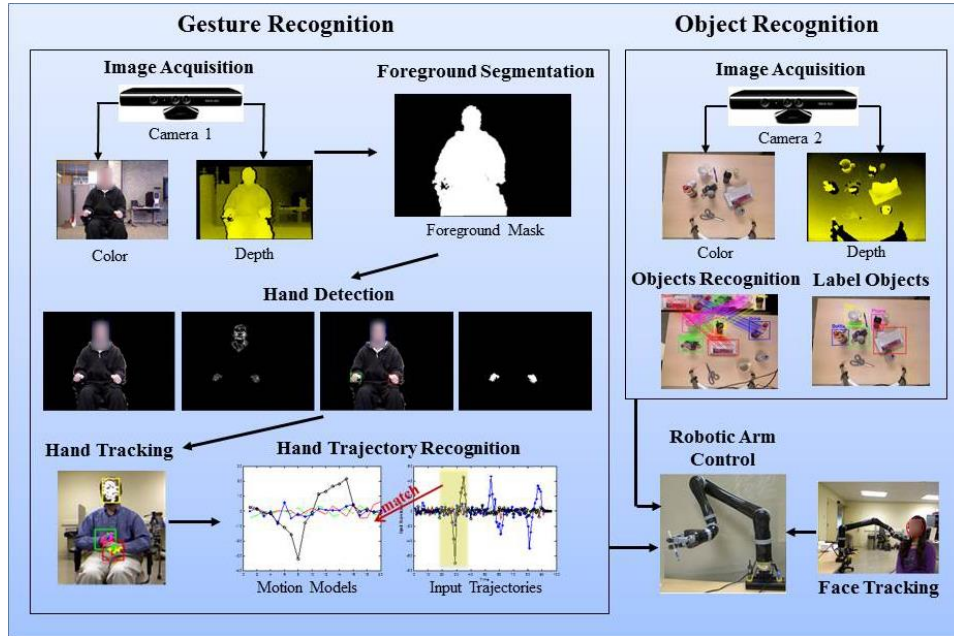


Fig. 1. System Architecture

In our previous studies (Jiang *et al.*, 2012a), a gesture recognition-based interface was designed and developed to allow individuals with upper-level SCIs to send commands for robotic control. In this paper, we combine this gesture recognition-based interface with face and object recognition modules for subjects to more efficiently retrieve daily living objects (Pirsiavash and Ramanan, 2012) in the environment. This study allows for further investigation of this completely vision-based WMRM controller.

2. System Architecture

The architecture of the proposed system is illustrated in Figure 1. Two Kinect® (Yanik *et al.*, 2012) video cameras were employed and served as inputs for the gesture recognition and object detection modules respectively. One camera is mounted to the wheelchair and faced to the subject for gesture recognition and face detection, and the other camera is faced down to recognize the objects. The results of these two modules were then passed as commands to the execution modules to control the JACO robotic arm (Kinova, Inc., Montréal, Canada). Briefly, these modules are described as follows:

2.1. Gesture Recognition Module

The video input from Kinect camera was processed in four stages using for gesture recognition based WMRM system control; foreground segmentation, hand detection, tracking, and hand trajectory recognition stage. Foreground segmentation was used to

increase computational efficiency by reducing search range for hand detection and later stage process. The face and hands were detected from the foreground which provided an initialization region for hand tracking stage. The tracked trajectories were then segmented and compared to the pre-constructed motion models and classified them as certain gesture groups. The recognized gesture was then encoded and passed as command to control the WMRM.

2.2. Object Recognition Module

The goal of the object recognition module is to detect the different daily living objects and assign a unique identifier for each of these objects. A template was created for each object being recognized. These templates were compared to each frame in the video sequence to obtain the best matching object. The results were then encoded and passed as commands to position the robotic manipulator.

2.3. Automatic Face Detection Module

A face detector (Viola and Jones, 2001) was employed in this module to perform automatic face detection. The goal was to provide a shortcut for the subjects to position the objects to the front of the face by controlling the robotic arm.

2.4. Execution Module

The robotic arm was programmed as a wrapper using JACO API under C# environment which was then called by the main program. The JACO robotic arm was mounted to the seat frame of a motorized wheelchair. The robotic arm was controlled by the encoded commands from gesture recognition, automatic face detection and object recognition module.

3. Methodology

3.1. Gesture Recognition-Based Interface

In this section, a brief introduction is provided for the gesture recognition-based interface (Figure 1. left column). A detailed description can be referred to (Jiang *et al.*, 2012a, 2012b).

3.1.1. Foreground Segmentation

Two steps were adopted in this stage to segment the human body and its connected components (i. e, the wheelchair) as the foreground. In the first step, the depth information was acquired by a Kinect sensor with depth value $D(i, j)$ for each pixel, where, i and j denote the horizontal and vertical coordinates of the pixel. Each frame was then thresholded by the depth value of each pixel. Two thresholds (T_{DH} and T_{DL}) were set to remove the pixels outside this range (Jiang *et al.*, 2012b). Only those pixels with a depth value between T_{DH} and T_{DL} were kept in a binary mask image. In the second step,

the largest region was extracted as the foreground and all the remaining blobs with a smaller area were discarded. The largest region contains not only the human body, but also its connected components.

3.1.2. Hand Detection and Tracking

Skin color detection was conducted by employing two 3D histogram models. A face detector (Viola and Jones, 2001) was used to remove the face region and extract the remaining two largest blobs as the hand regions. The face and hands detection results were only used to provide an initialization region for hand tracking. A three dimensional particle filter framework was employed to track the hands through all the video sequence by incorporating both color and depth information. In addition, an interaction model using motion and spatial information was integrated to the particle filter framework to solve “false merge” (when the tracker loses the object being tracked and mistakenly focuses on a different object that has higher observation likelihood) and “false labeling” (when exchange of labels assigned to objects after interaction or occlusion occurs). These problems usually occur when hands cross or overlap each other (Jiang *et al.*, 2012a, 2012b).

3.1.3. Trajectory Recognition

An eight-gesture lexicon (Figure 2) was adopted for the gesture recognition based interface (Jiang *et al.*, 2012a). The acquired hand positions from the tracking stage were then formed as trajectories and compared with the motion models of each gesture in the lexicon. The motion models were created by using the training data collected from eight able-bodied and two subjects with quadriplegia. The training data was then aligned using the dynamic time warping algorithm (Aach and Church, 2001). The CONDENSATION algorithm (Black and Jepson, 1998) was then used to recognize the input gesture trajectories. The state S at time t was extended to be used for two hand gestures as Equation (1):

$$S_t = (\mu, \varphi^i, \alpha^i, \rho^i) = (\mu, \varphi^{right}, \varphi^{left}, \alpha^{right}, \alpha^{left}, \rho^{right}, \rho^{left}). \quad (1)$$

where, μ is the index of the motion models, φ is the current phase in the model, α is an amplitude scaling factor, ρ is a time dimension scaling factor, i equals to right hand, or left hand. Each classified gesture was then passed as commands to control the WMRM. As mentioned in (Tsui *et al.*, 2011) this gesture recognition based interface can provide a recognition accuracy of 95.8%.

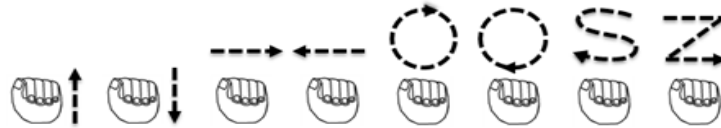


Fig. 2. Gesture lexicon. (a) upward; (b) downward; (c) rightward; (d) leftward; (e) clockwise circle; (f) counter-clockwise circle; (g) figure S; (h) figure Z.

3.2. Object Recognition

An object recognition module was developed concurrently with the gesture recognition-based interface to provide more efficient operation for quadriplegic users in retrieving objects (Figure 1, right column). Each frame of the video sequences was captured by a Kinect camera. The distance of each pixel within an object from the depth sensor was mapped to intensity levels. Thus, the nearer the object is from the sensor, the higher the intensity is. An example of the color and depth frames is shown in Figure 3. In this figure, different daily living objects that a wheelchair user would be expected to often retrieve and bring to one's face were tested, including a box of tissues, cordless telephone, water bottle, coffee mug, and electric shaver. In addition, these objects vary significantly in shape, size, and weight for more exhaustive testing of object recognition and robotic arm manipulation.



Fig. 3. (a) Color frame of test objects (b) Depth frame of test objects.

A Speeded Up Robust Features (SURF) algorithm was employed to recognize these daily living test objects (Bay *et al.*, 2006). A template with SURF features for each object was created before the object recognition process. Each frame captured by the Kinect camera was passed as input to the object recognition system. The SURF algorithm was then applied to each frame to acquire the features. These obtained features were then compared to the template features to get the best matching point pairs which were used to localize the objects (Figure 4). The label for each object was given to the matching object. Since SURF is a feature matching algorithm, a template of each object of interest needs to be acquired and properly annotated for future recognition. Then, a dictionary was constructed including the aforementioned templates. The templates include a: (a) box of tissues, (b) cordless telephone, (c) water bottle, (d) coffee mug, and (e) electric shaver.

After localizing the objects, the robotic manipulator could be automatically directed to the position of the object. However, in this study we did not tackle the problem of how to grab random objects. The objects selected for grabbing was from the pre-built library.

In terms of these constraints, the robotic arm needed to be fixed in a position where the object was not touched. The highest point of the object was extracted by computing the smallest value within the detected object region in the depth frame. This object recognition and localization process is called “coarse localization”. In this paper, “fine localization” for object grasping and manipulating were accomplished by hand gesture recognition-based control.

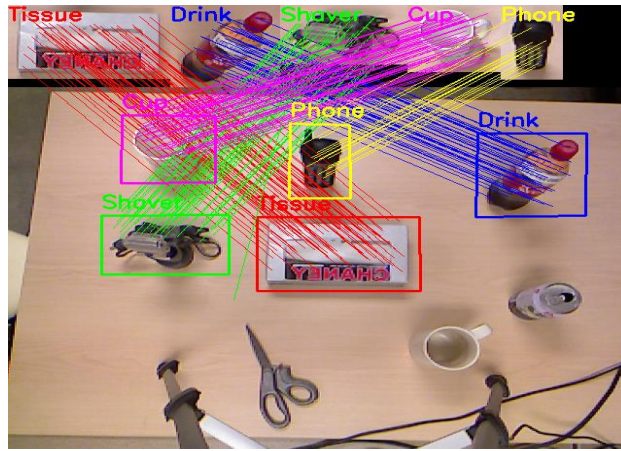


Fig. 4. Automatic Recognition of Daily Living Objects.

3.3. Robotic Manipulator Control Policies

The JACO robotic manipulator was mounted on the left side of the wheelchair (Figure 5(a)) to provide users with disabilities more capabilities to interact and manipulate the objects in the environment (Figure 5(b)). The JACO robotic arm was manufactured specifically to be mounted on wheelchairs to assist users in performing manipulation tasks. A C# wrapper was implemented using the resident JACO API to control the robotic manipulator. The JACO robotic manipulator has 6 degrees of freedom that were separated into three control modes: 3-D translation of the hand, wrist rotation, and finger grasping. During operation each mode had to be selected. Under translation and wrist control mode, three axes were controlled. Under finger control mode, two or three finger grasping could be selected. The eight-gesture lexicon in Figure 2 was used to control the system. A mapping between the gestures and the robotic control modes are shown in Table II.

Table II. Gesture controls for the robotic arm.

Gesture	JACO Arm Control Mode		
	Translation (Directional hand motion)	Wrist	Finger
Upward	Up	Wrist rotation (clockwise)	--
Downward	Down	Wrist rotation (counter-clockwise)	--
Rightward	Right	Lateral orientation (index side)	Open three fingers
Leftward	Left	Lateral orientation (thumb side)	Close three fingers
Clockwise Circle	Forward	Vertical orientation (top side)	Open two fingers
Counter-clockwise Circle	Backward	Vertical orientation (bottom side)	Close two fingers
Z	Change mode (translation to wrist)	Change mode (wrist to translation)	Change mode (finger to wrist)
S	Change mode (translation to finger)	Change mode (wrist to finger)	Change mode (finger to translation)

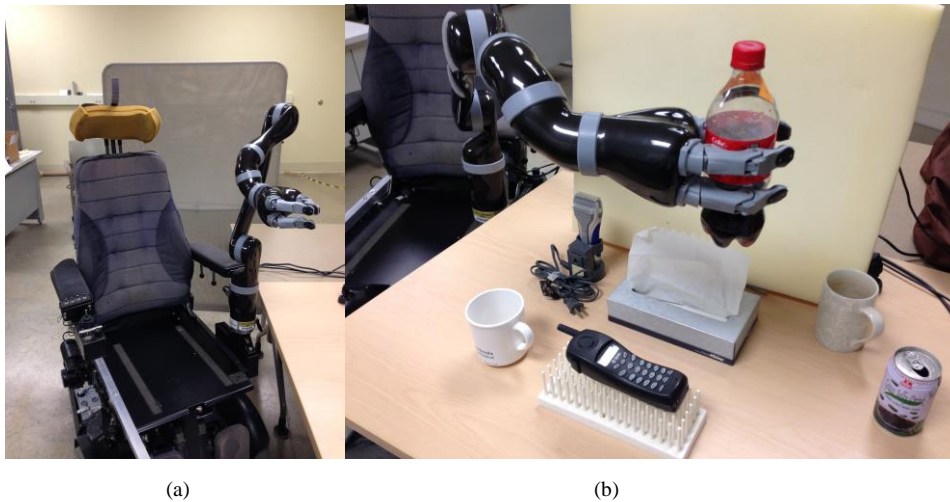


Fig. 5. (a) JACO robotic arm (b) Object manipulation.

3.4. Robotic Manipulator Control Policies

The robotic manipulator could be controlled through the integration of the gesture recognition-based interface, object recognition module, and automatic face detection. The gesture recognition controller was used to operate the robotic manipulator for fine localization. The object recognition and face detection modules were used for coarse localization of the robotic arm to the selected object and the user’s face to provide more

efficient robotic arm control. This flow chart of the proposed system is described in Figure 6.

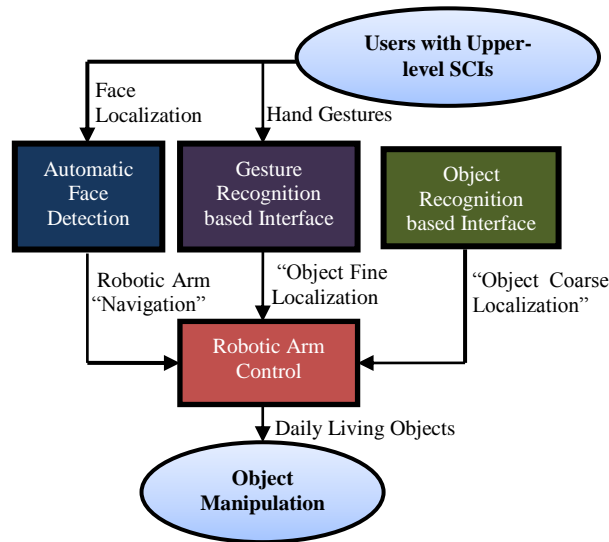


Fig. 6. Integrated computer vision system flow chart

4. Experiments and results

Preliminary experimentation was conducted with three able-bodied subjects to demonstrate the validity of the system. The Institutional Review Board (IRB) approval has been obtained to conduct this study. Although no subjects with upper-level spinal cord injuries were recruited in this experiment section, the gesture lexicon was constructed with three subjects with upper extremity mobility impairments and the gesture recognition based control system has already been evaluated with two subjects with quadriplegia (Jiang *et al.*, 2012a, 2012b). In this paper, we plan to test a more efficient means to operate a WMRM using the proposed optimized vision-based system. Five daily living objects (box of tissues, coffee mug, electric shaver, cordless phone and 16 ounce drink bottle) were selected as test targets to be manipulated by the vision-based system. These test objects were selected based on their variety of shapes, sizes, and weights. Two sets of performance experiments were compared. One is the "Manual" control experiment, which was to have subjects only use gestures to position the robotic manipulator to a test object, pick up the object, and position it in front of the face of the subject. The other experiment is "Semi-automatic" control, which was to perform object recognition to position the robotic arm to the top of the test objects and then use hand gestures to perform "fine positioning" and picking up the object. Then automatic face

detection was used to position the object in front of the subject’s face. The gesture lexicon in Figure 2 was used in this section for robotic arm control (Figure 7).

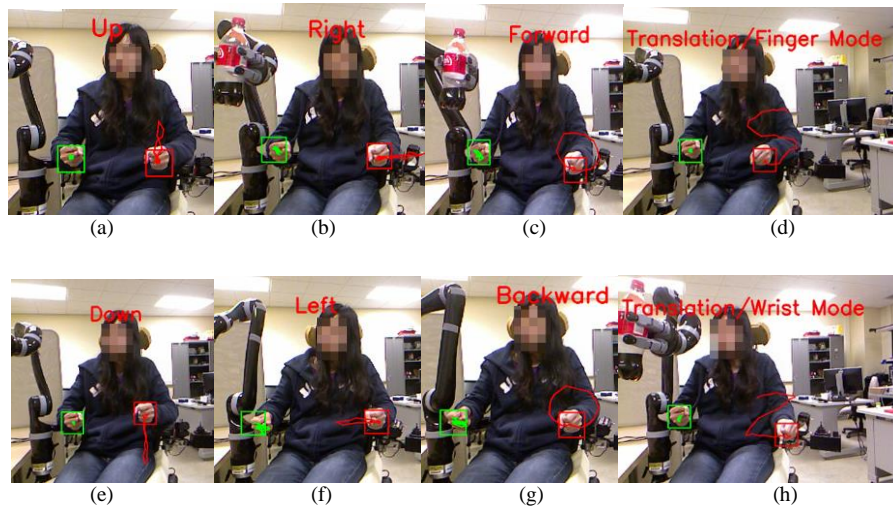


Fig. 7. Gesture recognition based robotic control sample results. (a) up; (b) right; (c) forward; (d) change mode (translation to finger mode); (e) down; (f) leftward; (g) backward; (h) change mode (translation to wrist mode).

The average task completion time (mean with variance) for object grasping was compared (Figure 8). As expected, there was a significant difference between the average task completion time of “Semi-automatic” (176.9s) and “Manual” (287.4s) control.

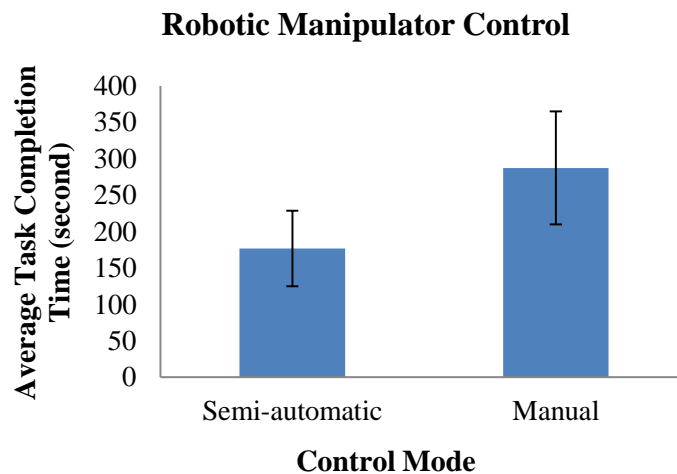


Fig. 8. Comparison between semi-automatic and manual robotic manipulator control modes, single factor ANOVA, $p < 0.05$.

Average task completion time (mean with variance) for particular objects were also performed (Figure 9). There was no significant difference in task completion times among different objects. However, for the objects as cordless phone, since it needed to be grasped without touching the keyboard, the subjects may need more time to figure out a proper orientation to move towards it under “manually control”. While under “Semi-automatic” control, the robotic arm was already located above the object, so the subjects only need to rotate the robotic arm with a few operations and then move the robotic arm down to grasp the cordless phone which cost them less time.

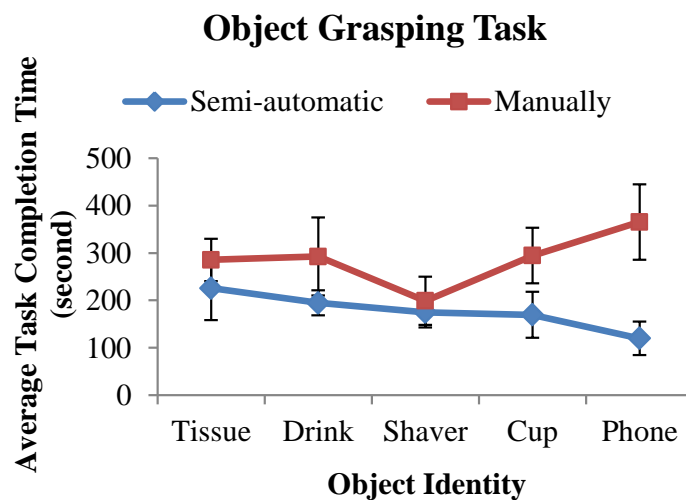


Fig. 9. Comparison among different object grasping tasks, single factor ANOVA, $p < 0.05$.

5. Discussion

This paper presents a pilot study of an integrated vision-based WMRM system that uses only gesture recognition or a combination of gesture recognition and automated object detection. In this section, the limitations of the gesture recognition and object detection algorithms, and experimental results are discussed.

Since the centroids of the face and hands were detected by applying the skin and non-skin color histogram models, several limitations exists. First, the system works for a single user and the performance of the system may be affected when the user wear short sleeves. More users appearing simultaneously in front of the camera may result in errors for the gesture recognition process. In addition, it is expected that the system was enabled when the users sit in the wheelchair.

The SURF algorithm was applied for objects recognition. SURF can be used for detection once it was previously trained with a dataset of instances of the same object under different conditions/configuration. For this reason, it can only be applied to known

objects. For recognition of unknown objects, one shot learning techniques can be used (Fei-Fei et al., 2006; Jiang et al., 2013a). To speed up the algorithm for real-time object recognition, GPU-based SURF can be applied, and this will be the subject of future work.

Two sets of experiments were conducted to test the feasibility of the system: “Manual” and “Semi-automatic” control. The two types of control took users an average of 287.4s and 176.9s, respectively, to accomplish object retrieval tasks. The average time includes: the users’ fine motor operation, the gestural commands’ recognition and the robot’s reaction time. Assuming we cannot speed up the user’s manual operation of the robotic arm, the more effective solution has been to apply automatic detection algorithms to reduce the task completion time. By applying algorithms to automatically grab objects according to their geometric characteristics, we were able to reduce the time and user effort required to perform largely course movements of the robotic arm. Joystick and keyboard manual control of the JACO robotic arm by quadriplegics has shown to be both mentally (making errors) and physically tiring when performing typical targeting and pouring tasks. In addition, the standard joystick that came with the JACO robotic arm was inaccessible to some quadriplegics due to fine motor impairments in their hands (Jiang *et al.*, 2013b). We believe this integrated vision-based control for the robotic arm will be both more accessible and less time-consuming than standard control modalities.

6. Conclusions and Future Work

This paper demonstrates the feasibility and greater efficiency of a WMRM control system that implements an integrated gesture recognition-based interface, compared to traditional interfaces for control. The algorithm used includes both face and object recognition capabilities.

An eight-gesture lexicon was employed and mapped to the robotic control functions. The gesture recognition-based interface provides individuals with high level SCIs a noninvasive method to control a WMRM and interact with objects around them.

The object recognition module simplified the process of robotic arm navigation and reduced the task completion time for object grasping. The face detection module provided the subjects with a shortcut to move the robotic arm towards the face instead of manually localizing and directing the robot towards it. It was shown that this “semi-automatic” mode saves users time and labor in performing common retrieval tasks, which would be the bulk of activity for a WMRM.

Moreover an “automatic” mode may further reduce the time for individuals with SCIs to control the robotic arm, but also it would constrain the user’s control and flexibility. The “semi-automatic” control mode is a good compromise between these two conflicting objectives and serves as an optimal solution. The semi-automatic mode saves time and effort for the users and at the same time provides them with more flexibility in robotic arm control for object manipulation.

Future work will include; (1) recruiting more subjects, particularly those with upper-level SCIs, (2) integrating the whole system in a more efficient and practical design for

practical use for wheelchair users, and (3) improving object recognition algorithm to allow the robotic arm to grasp objects according to their affordance.

Acknowledgments

This work was performed at the Institute for Accessible Science through the NIH Director's Pathfinder Award to Promote Diversity in the Scientific Workforce, funded by the American Recovery and Reinvestment Act and administered by the National Institute of General Medical Sciences (grant no. 1DP4GM096842-01). We are grateful for the assistance of Jamie Nolan from the Institute for Accessible Science and Mithun Jacob from the Intelligent System and Assistive Technology (ISAT) lab at Purdue University.

References

- Aach, J. and Church, G. M. (2001). Aligning gene expression time series with time warping algorithms. *Bioinformatics*, **17**: 495–508.
- Amat, J. (1998). Intelligent wheelchairs and assistant robots. *Autonomous Robotic Systems*, Springer London, 211–221.
- Bailey, M. and Chanler, A. Maxwell, B. Micire, M. Tsui, K. Yanco, H. (2007). Development of Vision-Based Navigation for a Robotic Wheelchair. In: *IEEE 10th International Conference on Rehabilitation Robotics (ICORR)*, 951–957.
- Bay, H. and Tuytelaars, T. Gool, L. V. (2006). SURF: Speeded Up Robust Features. *Computer Vision – ECCV 2006*, Springer Berlin Heidelberg, 404–417.
- Black, M. J. and Jepson, A.D. (1998). A probabilistic framework for matching temporal trajectories: Condensation-based recognition of gestures and expressions. *Computer Vision — ECCV'98*, Springer Berlin Heidelberg, 909–924.
- Chung, C.-S. and Cooper, R. A. (2012). Literature Review of Wheelchair-Mounted Robotic Manipulation: User Interface and End-User Evaluation. In: *RENA 2012 Annual Conference*. Baltimore, MD, USA.
- Eftring, H. and Boschian, K. (1999). Technical results from Manus user trials. In: *ICORR '99: International Conference on Rehabilitation Robotics*, Stanford, CA, USA.
- Fei-Fei, L. and Fergus, R. Perona, P. (2006). One-shot learning of object categories. *IEEE Transactions on Pattern Analysis and Machine Intelligence*, **28**: 594–611.
- Hashimoto, M. and Takahashi, K. Shimada, M. (2009). Wheelchair control using an EOG- and EMG-based gesture interface. In: *IEEE/ASME International Conference on Advanced Intelligent Mechatronics (AIM)*, 1212–1217.
- Hemmerling, T. M. and Taddei, R. Wehbe, M. Zaouter, C. Cyr, S. Morse, J. (2012). First robotic tracheal intubations in humans using the Kepler intubation system. *British Journal of Anaesthesia*, **108**: 1011–1016.
- Jacko, J. A. (2011). Human-Computer Interaction Design and Development Approaches. In *14th HCI International Conference*, 169–180.
- Jiang, H. and Duerstock, B. S. Wachs, J. P. (2012a). Integrated gesture recognition based interface for people with upper extremity mobility impairments. In *Proceeding of the 4th International Conference on Applied Human Factors and Ergonomics*.
- Jiang, H. and Duerstock, B. S. Wachs, J. P. (2013a). A Machine Vision-Based Gestural Interface for People With Upper Extremity Physical Impairments. *IEEE Transactions on Systems, Man, and Cybernetics: Systems Early Access Online*.
- Jiang, H. and Wachs, J. P., Duerstock, B. S. (2012b). Facilitated Gesture Recognition Based Interfaces for People with Upper Extremity Physical Impairments. *Progress in Pattern Recognition, Image Analysis, Computer Vision, and Applications*, Lecture Notes in Computer Science. Springer Berlin Heidelberg, 228–235.

- Jiang, H. and Wachs, J. P. Pendergast, M. Duerstock, B. S. (2013b). 3D joystick for robotic arm control by individuals with high level spinal cord injuries. *In: Proceedings of IEEE International Conference on Rehabilitation Robotics*, Seattle, June 24-26.
- Kim, D.-J. and Hazlett-Knudsen, R. Culver-Godfrey, H. Rucks, G. Cunningham, T. Portee, D. Bricout, J. Wang, Z. Behal, A. (2012). How Autonomy Impacts Performance and Satisfaction: Results From a Study With Spinal Cord Injured Subjects Using an Assistive Robot. *IEEE Transactions on Systems, Man and Cybernetics, Part A: Systems and Humans*, **42**: 2–14.
- Kim, D.-J. and Lovelett, R. Behal, A. (2009). An empirical study with simulated ADL tasks using a vision-guided assistive robot arm. *In: IEEE International Conference on Rehabilitation Robotics (ICORR)*, 504–509.
- Maheu, V. and Frappier, J. Archambault, P. S. Routhier, F. (2011). Evaluation of the JACO robotic arm: Clinico-economic study for powered wheelchair users with upper-extremity disabilities. *In: 2011 IEEE International Conference on Rehabilitation Robotics (ICORR)*, 1–5.
- Moon, I. and Lee, M. Ryu, J. Mun, M. (2003). Intelligent robotic wheelchair with EMG-, gesture-, and voice-based interfaces. *In: 2003 IEEE/RSJ International Conference on Intelligent Robots and Systems (IROS)*, **3**: 3453–3458.
- Nishimori, M. and Saitoh, T. Konishi, R. (2007). Voice controlled intelligent wheelchair. *In: SICE, 2007 Annual Conference*, 336–340.
- Palankar, M. and De Laurentis, K. J. Alqasemi, R. Veras, E. Dubey, R. Arbel, Y. Donchin, E. (2009). Control of a 9-DoF Wheelchair-mounted robotic arm system using a P300 Brain Computer Interface: Initial experiments. *In: IEEE International Conference on Robotics and Biomimetics (ROBIO)*, 348–353.
- Park, K.-H. and Bien, Z. Lee, J.-J. Kim, B. K. Lim, J.-T. Kim, J.-O. Lee, H. Stefanov, D. H. Kim, D.-J. Jung, J.-W. Do, J.-H. Seo, K.-H. Kim, C.H. Song, W.-G. Lee, W.-J. (2007). Robotic smart house to assist people with movement disabilities. *Auton Robot*, **22**: 183–198.
- Pirsiavash, H. and Ramanan, D. (2012). Detecting activities of daily living in first-person camera views. *In: 2012 IEEE Conference on Computer Vision and Pattern Recognition (CVPR)*, 2847–2854.
- Reale, M. and Liu, P. Yin, L. (2011). Using eye gaze, head pose, and facial expression for personalized non-player character interaction. *In: 2011 IEEE Computer Society Conference on Computer Vision and Pattern Recognition Workshops (CVPRW)*, 13–18.
- Simpson, R. C. (2005). Smart wheelchairs: A literature review. *Journal of Rehabilitation Research and Development*, **42**: 423–435.
- Tsui, C. S. L. and Jia, P. Gan, J. Q. Hu, H. Yuan, K. (2007). EMG-based hands-free wheelchair control with EOG attention shift detection. *In: IEEE International Conference on Robotics and Biomimetics (ROBIO)*, 1266–1271.
- Tsui, K. M. and Kim, D.-J. Behal, A. Kontak, D. Yanco, H. A. (2011). “I want that”: Human-in-the-loop control of a wheelchair-mounted robotic arm. *Applied Bionics and Biomechanics*, **8**: 127–147.
- Vaidyanathan, R. and Chung, B. Gupta, L. Kook, H. Kota, S. West, J. D. (2007). Tongue-Movement Communication and Control Concept for Hands-Free Human ndash;Machine Interfaces. *IEEE Transactions on Systems, Man and Cybernetics, Part A: Systems and Humans*, **37**: 533–546.
- Viola, P. and Jones, M. (2001). Rapid object detection using a boosted cascade of simple features. *In: Proceedings of the 2001 IEEE Computer Society Conference on Computer Vision and Pattern Recognition (CVPR)*, **1**:511–518.
- Wachs, J. P. and Stern, H., Edan, Y. (2005). Cluster labeling and parameter estimation for the automated setup of a hand-gesture recognition system. *IEEE Transactions on Systems, Man and Cybernetics, Part A: Systems and Humans*, **35**: 932–944.
- Wang, H. and Grindle, G. G. Candiotti, J. Chung, C. Shino, M. Houston, E. Cooper, R. A. (2012). The Personal Mobility and Manipulation Appliance (PerMMA): A robotic wheelchair with advanced mobility and manipulation. *In: 2012 Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC)*, 3324–3327.
- Yanco, H.A. (2000). Shared User-computer Control of a Robotic Wheelchair System. *Doctoral dissertation*, Massachusetts Institute of Technology.

Yanik, P. M. and Manganelli, J. Merino, J. Threatt, A. L. Brooks, J. O. Green, K. E. Walker, I.D. (2012). Use of kinect depth data and Growing Neural Gas for gesture based robot control. *In: 2012 6th International Conference on Pervasive Computing Technologies for Healthcare (PervasiveHealth)*, 283–290.

Biography



Hairong Jiang received her B. S. degree in control science and engineering Harbin Institute of Technology, in 2008. Her M.S. degree in control science and engineering from Harbin Institute of Technology Shenzhen graduate school, in 2010. She is currently working toward her Ph.D. degree at the School of Industrial Engineering, Purdue University, USA. Her primary research interests include gesture recognition and assistive technology.



Juan P. Wachs is an Assistant Professor in the School of Industrial Engineering at Purdue University. He is the director of the Intelligent Systems and Assistive Technologies Lab (ISAT) and he is affiliated with the Regenstrief Center for Healthcare Engineering. He completed a postdoctoral training at the Naval Postgraduate School's MOVES Institute in the area of computer vision, under a National Research Council Fellowship from the National Academics of Sciences and he was awarded the Air Force Young Investigator Award 2013. His research interests include machine and computer vision, robotics, teleoperations, human robot interaction, and assistive technologies. Juan Wachs is a member of IEEE and the Operation Research Society of Israel (ORSIS). He has published in journals including IEEE Trans. Systems, Man, and Cybernetics, Journal of American Medical Informatics, Communications of the ACM, and the Journal of Robotic Surgery. He received his M. Sc. and Ph.D. in Industrial Engineering and Management from the Ben-Gurion University of the Negev.



Bradley S. Duerstock is the corresponding author
Email: bsd@purdue.edu

Bradley S. Duerstock is the Director of the Institute for Accessible Science and an Associate Professor of Engineering Practice in the Weldon School of Biomedical Engineering and School of Industrial Engineering at Purdue University. He received his B.S. degree in Biomedical Engineering at the School of Interdisciplinary Engineering and Ph.D. degree in Neurobiology at the College of Veterinary Medicine from Purdue University, West Lafayette, IN, USA. He was a postdoctoral research associate at the Center for Paralysis Research at Purdue. His research interests focus on the restoration of function after disability through assistive technologies, human robot interaction, and accessible design. Dr. Duerstock received the NIH Director's Pathfinder Award to Promote Diversity in the Scientific Workforce in 2010.